

Spectroscopy Performance Note

Understanding the Glow Discharge Source

The Sputtering Process


- The Glow Discharge Spectrometer (GDS) lamp provides a low pressure argon environment (typically 5-10 Torr) over the sample surface.
- A high negative potential (typically -800 to -1200V) is applied to the sample. The sample thus becomes the cathode.
- Spontaneously produced Argon ions (Ar^+) are accelerated across the anode/cathode gap by this potential.
- The collision of Ar^+ ions with argon gas molecules causes plasma formation and further production of Ar^+ ions. This plasma is called a glow discharge.
- Some of these high velocity Ar^+ ions reach the sample surface where they sputter (or mill out) materials uniformly from the sample substrate.
- Some of this sputtered material diffuses into the glow discharge plasma where it is dissociated into atomic particles and finally excited.
- The light emitted from these excited state species as they collapse back to a lower energy level is characteristic of the elements composing the sample.
- The wavelengths and intensity of the light emission are used to identify and quantify the composition of the sample.

GDS Advantages

- Layer-by-layer removal of material allows for qualitative and quantitative depth profile analysis
- Separation of sampling (sputtering) and excitation resulting in:
 - Freedom from metallurgical history
 - Fewer matrix effects
- Grimm-type Lamp design provides lowered self-absorption and material re-deposition
- Linear calibration curves with wide dynamic range
- Fewer lines required to analyze full concentration range
- Linear calibrations require fewer standards for calibration
- Fewer spectral interferences due to:
 - Narrow emission lines
 - Excitation of almost exclusively atom lines
- Very little sample-to-sample carry-over allows quick matrix changes
 - Automatic cleaning between samples
 - No sputtering of anode or other lamp components
- Low reference material consumption
 - More burns before required resurfacing
 - Shallower burn spots requiring less material removal during resurfacing
- Low gas and other consumable consumption
- Very easy to operate
- Quiet, clean, and low maintenance
- Small footprint—fits through standard lab door



GDS500A

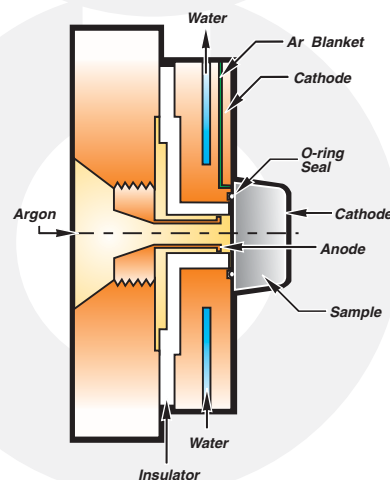

GDS Source



GDS Lamp



Delivering the Right Results

Form No. 209-076-035

LECO Corporation

3000 Lakeview Ave. • St. Joseph, MI 49085

Phone: 800-292-6141 • Fax: 269-982-8977

info@leco.com • www.leco.com • ISO-9001:2000 No. FM 24045

LECO is a registered trademark of LECO Corporation
6/07-REV0

© 2007 LECO Corporation